

jms:cca:down i-cholesteryl


# A4

Current Data Parameters  
NAME 24165142  
EXPNO 10  
PROCNO 1

F2 - Acquisition Parameters  
Date\_ 20131024  
Time 17.20  
INSTRUM spect  
PROBHD 5 mm PABBO BB/  
PULPROG zg30  
TD 65536  
SOLVENT CDCl3  
NS 8  
DS 0  
SWH 8012.820 Hz  
FIDRES 0.122266 Hz  
AQ 4.0894465 sec  
RG 197.36  
DW 62.400 usec  
DE 17.37 usec  
TE 295.9 K  
D1 1.00000000 sec  
TD0 1

===== CHANNEL f1 =====  
SFO1 400.1324710 MHz  
NUC1 1H  
P1 10.00 usec  
PLW1 27.20000076 W

F2 - Processing parameters  
SI 65536  
SF 400.1300000 MHz  
WDW EM  
SSB 0  
LB 0.30 Hz  
GB 0  
PC 2.00

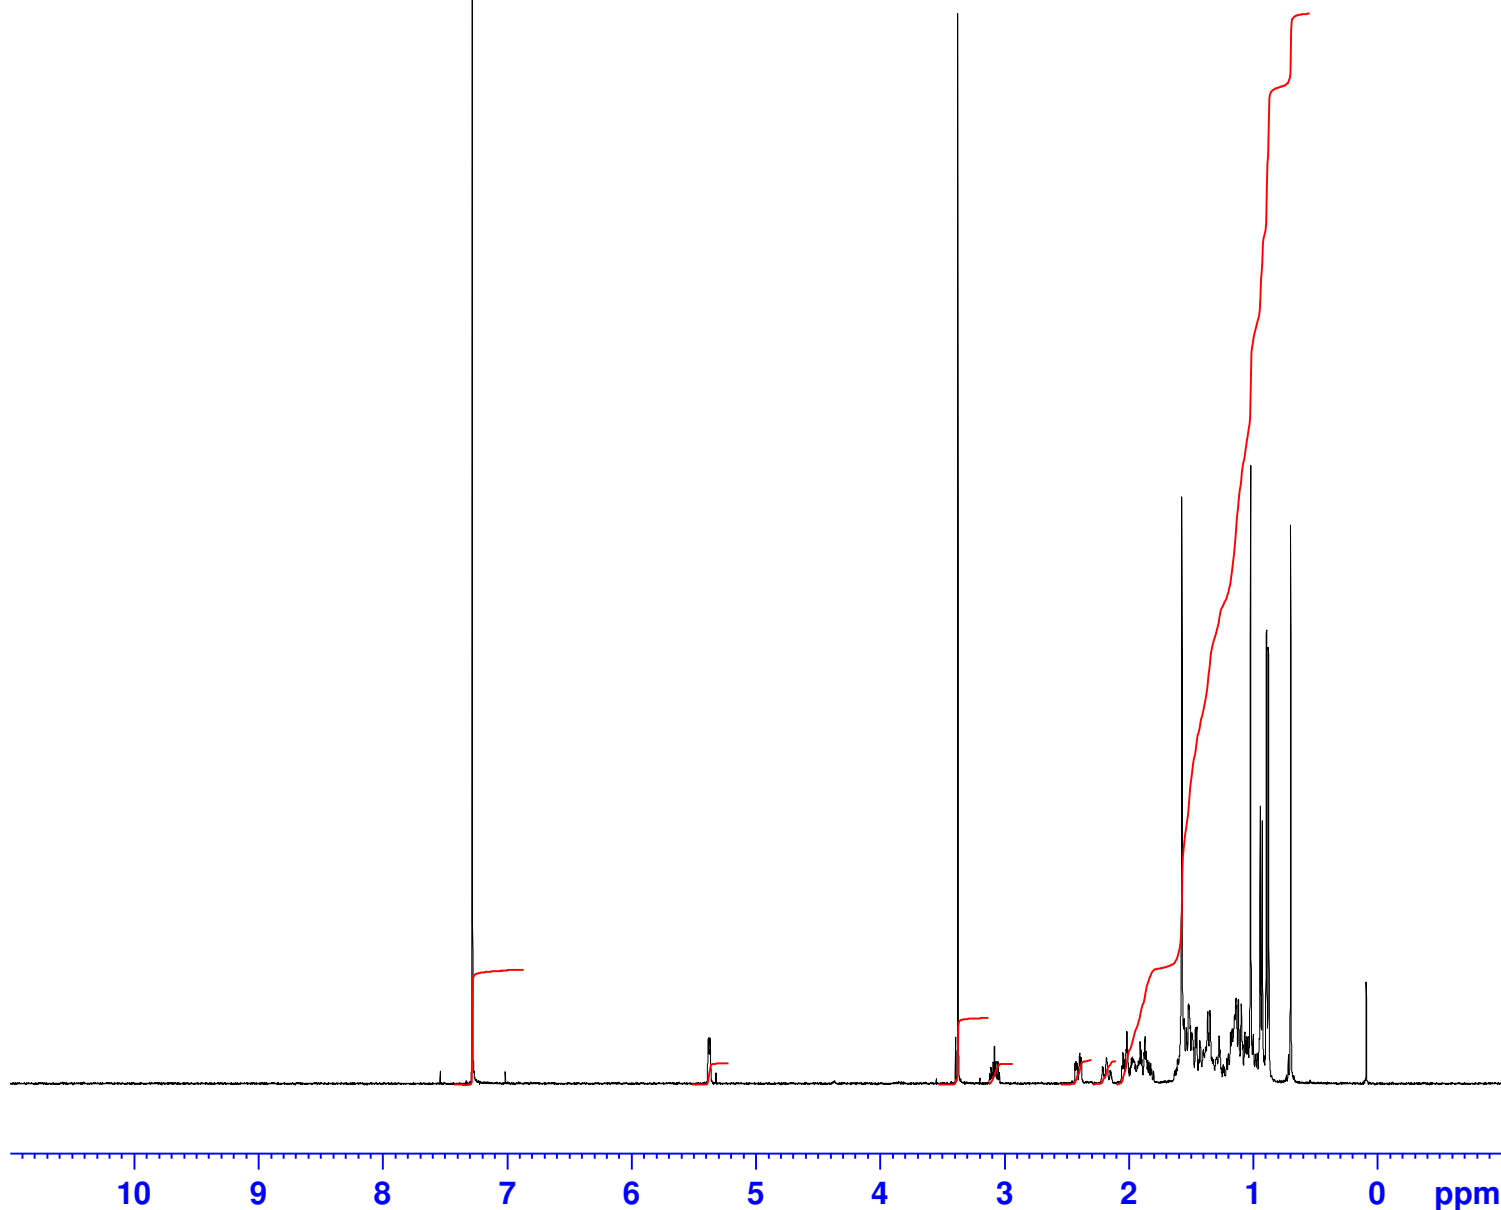

8.52

1.57

4.96

1.54

1.83

1.74

79.84