


B4

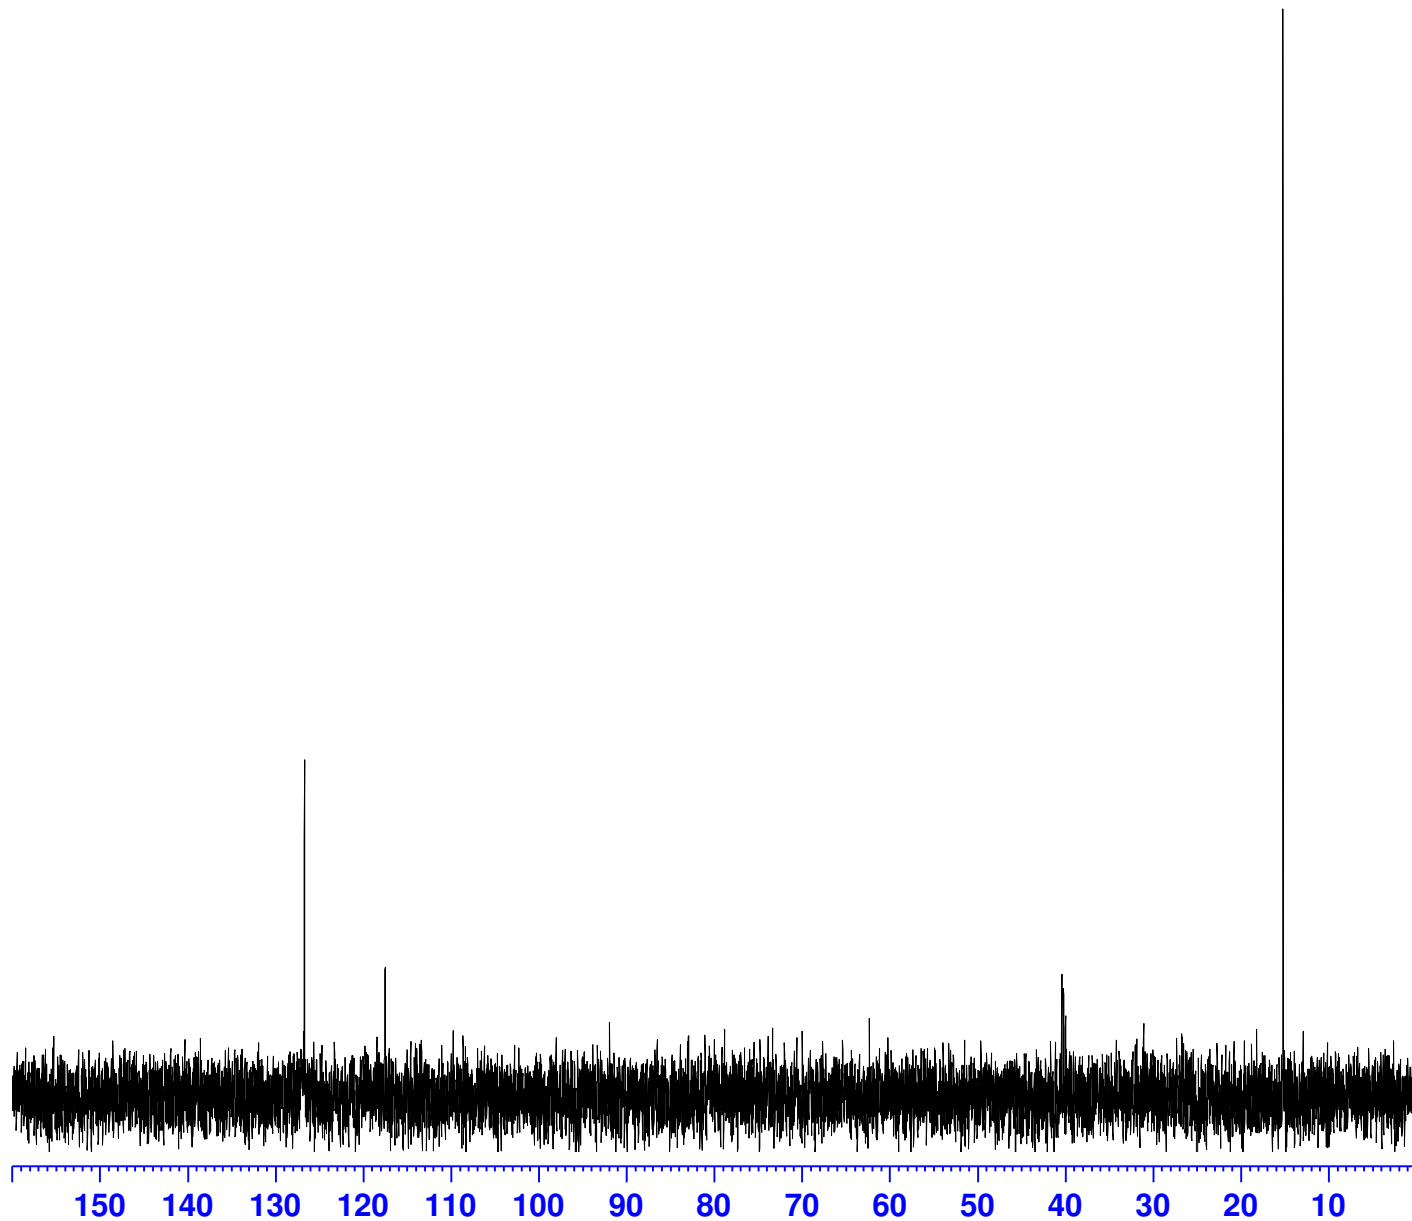

Current Data Parameters

NAME 03163431
EXPNO 11
PROCNO 1

F2 - Acquisition Parameters

Date_ 20140404
Time 0.26
INSTRUM spect
PROBHD 5 mm PABBO BB/
PULPROG deptsp135
TD 65536
SOLVENT DMSO
NS 128
DS 0
SWH 16129.032 Hz
FIDRES 0.246110 Hz
AQ 2.0316160 sec
RG 207.78
DW 31.000 usec
DE 9.84 usec
TE 297.3 K
CNST2 145.0000000
D1 2.00000000 sec
D2 0.00344828 sec
D12 0.00002000 sec
TD0 1

===== CHANNEL f1 =====

SFO1 100.6039681 MHz
NUC1 13C
P1 8.00 usec
P13 2000.00 usec
PLW0 0 W
PLW1 75.30000305 W
SPNAM[5] Crp60comp.4
SPOAL5 0.500
SPOFFS5 0 Hz
SPW5 7.36320019 W

===== CHANNEL f2 =====

SFO2 400.0642795 MHz
NUC2 1H
CPDPRG[2] waltz16
P3 12.20 usec
P4 24.40 usec
PCPD2 65.00 usec
PLW2 17.00000000 W
PLW12 0.59887999 W

F2 - Processing parameters

SI 32768
SF 100.5959210 MHz
WDW EM
SSB 0
LB 1.00 Hz
GB 0
PC 1.40